

Consultant
Training Centre
Calibration Services

CERTIFICATE OF CALIBRATION

Instrument Details:

Name : Thermometer Digital
Manufacturer : Fluke
Type/Model : 62 Max /Infrared
Serial Number/Code : 38401981WS
Capacity/Nominal/Range : 50 ~ 500 °C
Resolution : 0,1 °C

Page 1 of 2

Standard & Equipment:

Code : BMD-SH-BBC01
Traceable to SI through : LK-160-IDN
Reference Method : Inhouse Procedure
Calibration Procedure : BMD/IK/7.2/SH/07

Testing Condition:

Location : In Lab
Date of Calibration : November 13th 2020
Temperature (°C) : 32 ± 0,6
Humidity (%) : 67,1 ± 2

Owner's Identification:

Name : PT. Sertifikasi Mandiri Sejahtera
Address : Komplek Golden Plaza Fatmawati Blok J27,Lt.2 JL.RS.Fatmawati No.15 Kel.Gandaria
Selatan Kec.Cilandak Jakarta Selatan 12420
Order Number : BMD-4391120

Note:

Calibration report and attachment available on next pages is an integral part of this certificate

Date of issue:


Tangerang Selatan, November 17th 2020

Certificate Number:

241.1120/TS1

Ir. Renaldo Moontri, MM

QC Manager

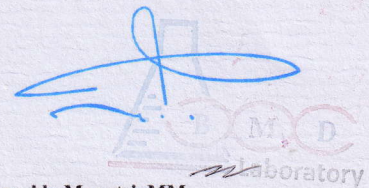

CALIBRATION RESULT

Instrument Details:

Certificate Number : 241.1120/TS1
 Name : Thermometer Digital
 Manufacturer : Fluke
 Type/Model : 62 Max /Infrared
 Serial Number/Code : 38401981WS
 Capacity/Nominal/Range : 50 ~ 500
 Unit Measurement : °C

Page 2 of 2

Temperature Setting °C	Instrument Reading °C	Correction °C	U 95 (±) °C
50	49,8	0,7	1,2
100	98,9	1,3	1,4
200	199,7	1,5	1,3
300	296,5	4,8	2,4
400	398,4	3,1	2,2
500	499,3	1,4	2,2

U 95% with coverage factor k = 2

Note : Emisivity Calibrator Standard 0,95

Calibrated by



(Muchlis Abdillah)

Calibration Officer



(Taofik Noor Alan)

Supervisor

